

Accessories for QXCI & SCIO

Operating Instructions

Probes, Rollers

Cellulite Rollers

Face and Pain Pads

Pet/Baby Pads

Water Energising Coil

Eye Attachment

Ear Attachment

Remedy Enhancer

BioEnergy Partnership
Supporting Quantum Users
Sales-Manuals-Training-Seminars

Contact: John Kelsey PhD


Email: info@qxcisynergy.co.uk

www.qxcisynergy.co.uk

Tel ++44 (0)121 243 6318

Fax ++ 44 0870 460 1138

27 Welcombe Grove, Solihull, England B91 1PD

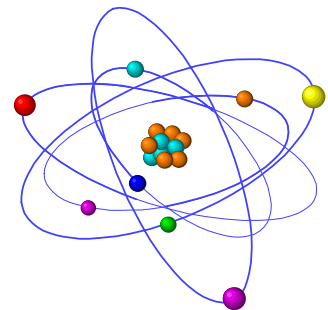

Contents

Updates	4
Part 1: Hardware	6
Hardware Introduction	6
Important Notes:	6
Principles in Outline	6
Application Overview	6
Guidance Notes	7
Power Settings, Frequency and Duration.....	8
Complete Treatments	8
Harness Activity.....	9
Optimizing the Treatments	9
Cleaning and Disinfecting.....	9
Cleaning	9
Disinfecting.....	10
Connection	11
For Treatment.....	11
For Testing.....	11
Standard Probe	12
Probe Accessories	12
D1: Spoon	12
D3: Extensor (straight).....	12
D5: Angled.....	12
Eye	12
Ear	12
Eye Treatment Accessory: Duplex	12
Principle of operation.....	12
The Experience that led to the development.....	13
Therapy Example	13
Ear Systems.....	14
Principle of operation.....	14
Standard Roller	14
Cellulite Roller.....	14
Cellulite Roller Oil Recipe.....	14
Pads	15
Pain, Beauty and Small Joint Pads.....	15
Remedy Enhancer-Potentiser.....	15
Cream Maker	15
Water Energising Coil.....	15
Splitter Box	17
Part 2: Program Facilities	18
Program Access Points	18
Deactivates the probe/roller	18
Test Screen Facilities	19
Dental.....	20
Tools	20

Functions Overview	20
Dental Therapies	20
TMJ Muscles.....	22
Tools	22
Test Screen facilities.....	22
TMJ Muscles.....	22
Pain	24
Tools	24
Program Facilities	24
Beauty: Body Scan and Face Therapy	25
Tools	25
Program Facilities	25
Sarcodes and Short Sarcodes (Eyes and Ears).....	27
General.....	27
Tools	27
Eyes: Main Treatment Locations	27
Sarcodes	27
Treatment Duration and Frequency	28
Basic Operation.....	28
Piggy backs- Additional Patterns.....	29
Short Sarcodes	29
Basic Operation.....	30
Short Sarcodes- Eyes	30
Short Sarcodes- Ears.....	31
Ear + etc.....	31
Piggy backs- Additional Patterns.....	31
Aging Program.....	32
Basic Operation.....	32
Other Therapy Places.....	33
Animals.....	34
Considerations specific to animals.....	34
Access	34
Pre-requisites.....	34
Specific Considerations for Horses.....	35
Basic Operation.....	35
General Screen	36
Physical foci.....	36
Potential causes.....	36
Nosodes and Isodes.....	36
Treatment	37
Potency Scan.....	37
Nutritional Intake	37
Part 3: Remedy making and Importation	39
Introduction.....	39
Important Notes:	39
Safety Note re Power Settings	40

Is the harness also active.....	40
Remedy Making.....	41
Preparation	41
Client in Harness- concurrent remedy and therapy.....	41
Client in Harness- remedy making only	41
Client not present	42
Alternative via Stimulate Reaction/Duplicate Remedy	42
Making remedies from the Main matrix: at matrix potencies.....	43
Making remedies from the Main matrix: with selected potency.	43
Selecting a potency.	43
Testing for Potency of a Main Matrix Item.	44
Testing for Potency of a Homeopathic Activation remedy	44
Multiple remedies	44
Importing remedy patterns (into the Test Matrix)	45
Procedure	45
Remedy Duplication	46
Test Screen (remedy duplication).....	46
Homeopathic Activation Screen (remedy duplication).....	47
Other Program Access Points	48
Test.....	48
Deactivates the probe/roller	48
Test Screen Facilities	49
Dental.....	49
Part 4: Product Information.....	51
Probes and Rollers	51
Oral use of Point Probe	52
Pain Pads.....	52
Eye Treatment Accessory	52
Pet-Baby-Large Area Pad	52
Cream Maker	53
Cellulite Roller.....	53
Water Energiser Coils.....	53

Updates

Please visit www.qxcisynergy.co.uk for latest releases.

June 2001 First Issue

April 2003

1. Disease lexicon also has point probe activate facility.
2. Cellulite Roller (heavy duty) available.
3. Beauty and Pain Pads available.
4. Animal/Baby Pad available.

October 2003 Issue 1.3

1. Eye and ear accessory added
Feb 2004 Issue 1.4
Rewrite

Part 1: Hardware

Hardware Introduction

Important Notes:

1. Whilst there are different devices they all connect in the same way.
2. Where probe is mentioned if appropriate to the treatment you can use the roller etc.
3. Be lateral and inventive.
4. Experiment with power settings (double) and duration of treatment and frequency of sessions: ***when using skin type treatments or energizing water set double power.*** When making energized water use double or max. power and do twice.

EXCEPT when using eye piece: use normal power

5. You can set the probe outlet in the test screen for all therapies from that time on to be output via the attachment as well as the harness.
6. Send me results..good or nothing.

Principles in Outline

In normal use the treatment waveforms are sent to the patient through the head harness. The energy must travel through the body to be used where it is needed. Localised treatment is possible when the head harness is placed near a focal area e.g. for the treatment of Fibrositis in the shoulder or a lesion when using the degeneration program.

The attachments enable the energy to be even more focused and thus potentially more effective. The power does not have so far to travel. A jet of water from a hose will clean an area on the wall of a swimming pool if it applied locally rather than having to travel through a mass of water first. Note however that this is not the whole picture: more is not necessarily better. The energy wave is subtle and it is the form rather than the power that is important. Applying locally means that the frequencies are not absorbed en route and more available for the specific aspect selected.

Within the test and dental screens it is possible to direct output to the point probe for any item in the test matrix. Within dental and Body Scan/Face Therapy specific therapies are available.

Application Overview

Some areas of application include:

Probe & Accessories

Dental: Infection
Small cavity repair assist
Gingivitis
General: any item from the test matrix
(3 sec or 3 min zap or zap from filter)
Mouth and tongue ulcers
Warts
Aging lines
Any therapy after the probe is activated in
the test matrix
Ears and eyes (special attachments)

Roller

Cellulite
General facial
General: any item from the test matrix
(3 sec or 3 min zap or zap from filter)
Larger skin areas for skin aging
Any therapy after the probe is activated in
the test matrix

Some ideas for the more specialist attachments include:

Cellulite Roller

Heavy areas of cellulite
Muscles

Pain & Beauty Pads

Any localized pain
Arthritic/painful small
joints

Animal/Baby Pad

Animals
Larger joints
Babies
Back pain

Guidance Notes

What you do depends on the condition.

Just follow the same logic that you would use for any issue that you are treating with the QXCI: based on understanding the process of the issue, the principle organs and systems involved.

Try treating for four minutes on each therapy and every three days for 2-3 weeks. Adjust according to results, generally to less frequent. Have clear markers in the real world and score each day. Reduce when there is a physical awareness of improvement then say once a month.

1. If there is a relevant test matrix item one way is to treat till the resonance decreases (in Individual Reaction), leave 3 days and retest before treating more.
2. If there is an absolutely confirmed medical diagnosis treat from this.
3. Respect the QXCI Test matrix, timed therapy, sarcodes etc. hints and treat
4. according to this also.
5. If there is an infective aspect identify and treat this. Use the hold tray facility to get associations.
6. Look at all the aspects involved in the issue: what systems are involved: treat these as well as the presenting issue. Try to approach the issue from a number of angles. E.g. general treatments for degeneration, injured tissue etc. as relevant.

7. Use the eye specific facilities in sarcodes, short sacodes and biofeedback with appropriate piggy back/additional treatment.

Power Settings, Frequency and Duration

The double power facility in the main test screen and dental has an effect on the probe. Please be safe and use appropriately. If you are using subtle treatments, the higher vibrational ones such as flower essences, homeopathics etc. then the attachments are less appropriate. The attachments are designed for localized application.

Try and identify markers that can be used with the Individual Reaction facility to monitor changes along with visual changes. Use digital photos where possible to document, especially for client!

All settings are just suggestions and should be adjusted according to child, elderly, vitality, severity etc. Monitor for patient discomfort/ alarm. If using head harness consider placing away from head e.g. abdomen (where there are as many brain cells!!)

There are specific suggestions in individual sections.

<i>Focus</i>	<i>Power</i>	<i>Frequency/Duration</i>
Eyes and ears	Normal	2-5 mins., x1-2 per week
Oral (Dental)	Double	2-5 mins., x1-2 per week
TMJ Muscles	Normal to double	2-5 mins., x1-2 per week
Pain, trauma	Double	As required.
Skin (beauty/aging)	Double	5-10 mins. x1-3 per week
Cellulite	Double	5-10 mins. x1-3 per week
Water Energising	Max.	Twice

Complete Treatments

Local treatments should be supported by supportive aspects, both within the QXCI and in real life. Local beauty treatments for example will be opposed by poor internal support. Beauty is reflective of the inside world as well. Not supporting this will mean that improvements won't show clearly or hold. In all cases, as in all dysfunctions, under the process and the stressors, helpers, organs and systems involved. The attachments are supportive accessories meant to be enhancements and not stand alone treatments. If there is no apparent success then look at what you are not doing to clear and support underlying issues.

Weight management: lymph, digestion, appropriate eating and exercise habits. . Support the relevant systems and organs.

Beauty: anti aging program, anti-oxidants, lifestyle stressors from the SOC etc. If working on the face if possible do a face diagnosis to check for any underlying issues. Either use a western or oriental face interpretation book or look at the basic hints in the QXCI (Face and Beauty>Oriental face Diagnosis). Support the relevant systems and organs. Consider using Sarcodes Therapy.

Pain: pain is a signal. Understand why the message is there and address the underlying aspects. Consider using Sarcodes Therapy.

Dental: infection-immune system, sugar, root canals, Mercury etc.

Harness Activity

The harness continues to stay active when the probe is active. The wave form goes through both outputs. Since the QX is putting out low energy wave forms, mainly of homeopathics, then the power is not reduced in the head harness channel. The inputs and auto-focus continues to operate. There is no need to remove the harness-this will also deliver the treatment so that any other parts of the client that want some of the healing pattern will benefit. There will be treatment effect through both routes: the harness is not disabled.

Optimizing the Treatments

- Remember that the client may experience that there is an issue but no pathology shows. There may be an energetic tendency that is felt but with no visible pathology. The following experience illustrates: *So, I made a homeopathic from the therapy of each eye part in the short sarcodes Rx page. I then tested myself against these homeopathics. The one I matched was Retina. So off I went to an optician and asked could he detect a cataract. Yes he could.*
- Make a supportive homeopathic using the potentiser: remove the harness, set max. power and export the pattern twice. Include any associated aspects such as circulation etc. that are relevant from the main matrix.

Cleaning and Disinfecting

Cleaning

To clean tarnished silver;

4 teaspoons of salt

4 teaspoons of baking soda (bicarbonate of soda)

Add to 1 litre of water, soak for 10 minutes, and dry with a soft cloth or a paper towel

Disinfecting

Restaurants clean utensils that go in our mouths in a dishwasher!

The options available include:


- Alcohol
- Cold sterilizing solutions as used in dental surgeries (available through medical supply houses)
- Autoclave: suitable for metallic parts only.

Connection

For Treatment

The devices plug into the red output on the rear of the harness interface box. The box must be connected to the computer and be powered (batteries or mains-adapter) for operation.

CONNECT TO THE RED ONLY

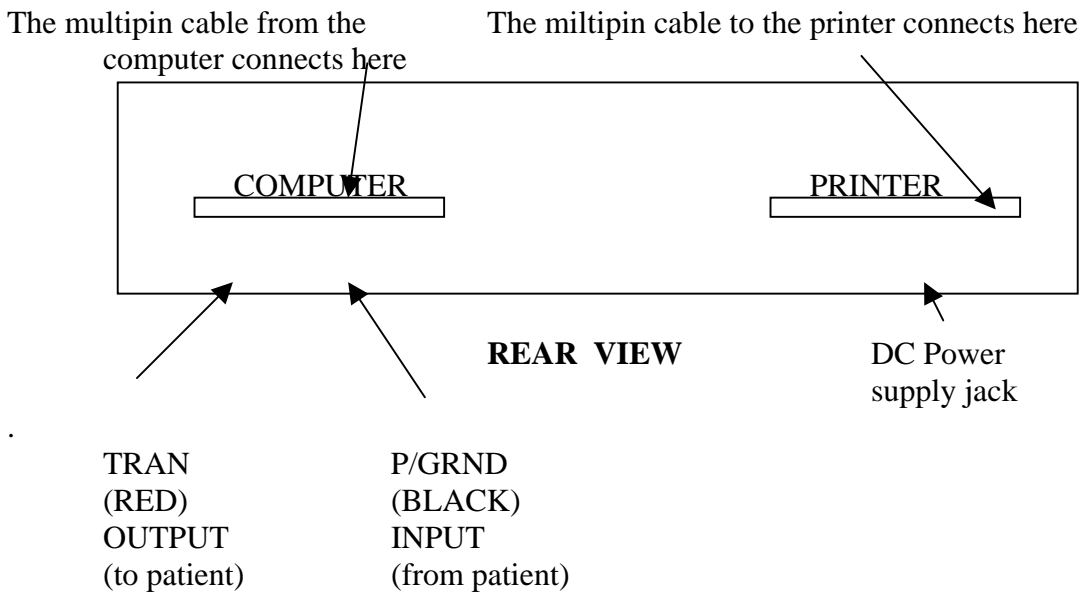

For Testing

The black input has been present on all QX harness boxes for using external remedy trays or in early devices an external test plate (integrated onto the white box in later versions as the metal panel on top). This is designed to test the patient reactivity to an item which is not in the test matrix.

IT IS NOT POSSIBLE AT PRESENT TO USE THIS INPUT FOR PROBE TESTING OF SPECIFIC LOCAL AREAS OR FOR GENERAL TESTING.

The attachments are designed for treatment: the normal test process should be used. For example when using the pet pad during the test the pattern of each item will pass through it BUT the response will be via the pick up straps. For animal or babies you may wish to test in subspace and treat using the attachments: the test results are theoretically 85% accurate in harness and 75% in subspace. The therapies are up to 400% stronger in harness. This does vary with the therapy: sarcodes, zaps etc. will generally be better in

harness. Biofeedback is soft and 90% subspace. Long undefined therapy option in many screens is subspace.

Standard Probe

The standard tip is general purpose and, from hygiene considerations, most appropriate for external use. The standard tip unscrews to allow other probe accessories to be screwed in.

Probe Accessories

D1: Spoon

Appropriate to larger surface blemishes than the point tips can fit. Also useful for internal ulcers, thrush, tongue etc.

D3: Extensor (straight)

Allows deeper penetration into the mouth for gum and muscle access.

D5: Angled

For tooth cavity zap/repair and between teeth. Can be used for under nail fungus.

Eye

The simplex attachment allows eye treatment through the closed lid at normal power. Also available as a duplex system with an electronics interface to ensure each eye receives treatment and no feedback between the eyes occurs.

Ear

Moulded to fit in ear. Also available as a duplex system mounting like headphones with an electronics interface to ensure each eye receives treatment and no feedback between the ears occurs

Eye Treatment Accessory: Duplex

Important Note

Undo the Knurled knob before adjusting the side arm: if you do not then the side arm can be damaged.

Principle of operation

The principle of operation is as for other attachments:

1. Connect to Red output from QXCI/SCIO to the green input on the interface box and then from this using the 2 red cables to the eye unit: one cable for each eye.
2. The Interface box MUST ALWAYS be used.
3. ALWAYS TREAT THROUGH THE EYELID: NOT ON THE OPEN EYE!!!
4. If you want to treat just one eye then use just one cable: it is not necessary to treat both eyes simultaneously, but you can.
5. Activate Point probe: Test>Treatments>Activate Point probe (it will then be active anytime that you want to use it)
6. The eyes are sensitive areas: it is suggested that you use normal power and 5-10 minute treatments every 2-3 days to establish a response pattern for that client.
7. The head harness and straps should be left in place: especially if you want to run tests.
8. As always look at the pathology of the issue and try to use the possible process to identify specific and general system intervention points.
9. If there is a confirmed medical condition then treat according to this.

The Experience that led to the development

My experience is that my left eye that was damaged in the past has improved quite a bit. I used to see for example a registration plate on a car as a jagged line rather than straight and the odd letter would be missing. Now all that is gone.

My right eye where I had a diagnosis of a cataract has improved a bit too. However I do not have a cataract that was a wrong diagnosis. I have a blocked vein in there. I am treating that now .I also use circulation and do Electro Chelation etc. etc. *I did do my eyes once on Max and the lids were all red the next day.*

Therapy Example

Example: occluded vein in the eye.

1. Timed therapies (sarcodes)- eyefollowed by the circulation button.
2. Circulation sarcode with electrochelaton etc and vein and artery buttons
3. Tmed therapies degeneration and injured tissue.
4. Go to the matrix and find the appropriate homeopathics and treat those too.
5. Look at the autonomic nervous systems in all conditions.
6. In this case as it is a blood vessel look at the Para because that mostly dilates.
7. If you have understanding of Chinese medicine use this also. For example Eye problems are of the WOOD Element so one would give therapy for that and of course treat the liver.
8. Make the homeopathic from the matrix.
9. Put all the therapies in a bottle (run the programs separately on Max. power without client in harness) along with the homeopathics

Ear Systems

Principle of operation

There are 2 sizes of ear attachment supplied: they can be used as a pair or for one ear only.

The principle of operation is as for other attachments:

1. Connect to Red output from QXCI/SCIO to the green input on the interface box and then from this using the 2 red cables to the ear unit: one cable for each ear.
2. The Interface box **MUST ALWAYS** be used when using a pair: this is to prevent feedback between eyes.
3. If you want to treat just one eye then use just one cable: it is not necessary to treat both ears simultaneously, but you can.
4. Activate Point probe: Test>Treatments>Activate Point probe (it will then be active anytime that you want to use it)
5. The ears are sensitive areas: it is suggested that you use normal power and 5-10 minute treatments every 2-3 days to establish a response pattern for that client. Depending on the issue involved then double power may be appropriate.
6. The head harness and straps should be left in place: especially if you want to run tests.
7. As always look at the pathology of the issue and try to use the possible process to identify specific and general system intervention points.
8. If there is a confirmed medical condition then treat according to this.

Standard Roller

This is a general purpose item suitable for external applications. It is applied firmly and evenly.

Cellulite Roller

This is a ribbed heavy duty item, suitable for more pronounced muscle and cellulite issues.

Cellulite Roller Oil Recipe

6 drops of Lavender oil

6 drops of Juniper oil

10 drops of Rosemary oil

Mix with 4 ounces (160 mls) of light vegetable oil

i.e. – Sunflower, Safflower or cold pressed Grape seed oil

Clean your Cellulite Roller with hot soapy water between patients

Note: Do not use Cellulite Oil with the Roller Assembly

Pads

Note: Face black side of animal pad to client

These are high conductivity rubber designed to transmit the pattern over larger areas. The size is selected to match the size of the organism or area to be treated.

Pads are available as follows:

- Babies, small pets, medium surface areas (e.g. back, thighs)
- Small children, medium pets (e.g. in a dog cage)
- Horses: under development)
- Couch mat

Pain, Beauty and Small Joint Pads

Up to 8 pads can be placed anywhere on the body. Secure with micropore or similar tape. Connect the back box to the red QXCI box via the red cable. Connect one or more of the pads via the smaller cables/ plugs into the black splitter box. Tape the pads into the desired positions and treat as normal.

Remedy Enhancer-Potentiser

Cream Maker

This is designed to distribute the pattern through an aqueous skin cream: any good non toxic water based cream will hold the pattern.

Water Energising Coil

These are in the shape of a coil to facilitate both left spin and right spin patterns, as an overlay on the ordinary energise water pattern. Right spin is intrinsic to health. The coil acts as a spin amplifier and correction facility. The spin varies between the Northern and Southern hemisphere. Perrier or Lourdes water, which carry particular energetic patterns because of their molecular structure, produced in the Northern hemisphere may not have benefits in the Southern hemisphere.

The following is intended to help the understanding of the benefits of water with good energetic patterns: this is not to say that chemically treated water is bad: indeed sterilization of water has saved many lives. Energising water optimizes its benefits.

Prof. P Nogier in Lyons, France developed the understanding that it is possible to examine the state of oscillation of every organ, from this evaluate the energetic circumstances of the organ and thus establish an equilibrium of oscillation. Water has a vital role in this in a conductor and storage medium for oscillations or energetic information. This facility is evidenced in homeopathic remedies.

Certain waters in nature are demonstrably beneficial: natural waters are more nurturing than “tap” water. Water that has been through pipes, pumps, treatment process and chemical additions has had the original natural energy and information compromised.

This may be threefold: additional undesirable patterns imparted to the water, loss of desirable patterns and also a locking up of the potential within the water. This latter aspects comes for the originator of the Q2/Befe unit: a water revitalising device. The foundation for this is that water contains intrinsically tremendous resources. In positive treatment we are not creating patterns but possibly facilitating release of water’s inner potential. Similarly unnatural treatment may put more impediment in the way of release of this potential.

The erasing of contaminant information and accessing the inner potential is the interest point. The process on nature provides one approach (and being of “nature”-al origin possibly the best. It has been observed that in the naturally correct flow of a river self purification occurs through the screw shaped, spiral turning of the water towards the centre. Measurements have been made to confirm that damaging frequencies can be erased by this motion. Thus even when drinking natures water the energetics may be lesser if the river has only a fast flow with a straight, smooth bed

In the case of chemical disruption the damaging frequencies will however tend to reappear: this highlights the need for a good quality water starting point.

Nature apparently uses physical spiral motion to create an energetic effect: within the water coil the spiral motion is imparted directly to the energetic output: the water will adopt this as equivalent to a natural process. This spiral aspect has also been observed in the arrangement of micro-organisms in some methods used to impart vitality to water.

This is the principle adopted in the coil: in addition to putting in homeopathic patterns that are intrinsically beneficial the spiral shape mimics nature to provide water with enhanced detoxification and rejuvenation benefits.

Test Results

A well known commercially available healing water was tested against quite a few differing devices and found it to be wanting. A local agent selling these units would not

accept than anything could be as good as his water. We gave him a sample of coil water and a sample of water that had been energised electronically. He took them away and returned with several marked bottles that included our two his and few others. When we ran our tests we had no idea which water was in which bottle. Much to his consternation our two gave the best results. This test was of course testing the readings of people against the each water sample. This is the only real test as far as I am concerned. We used separate devices from the QXCI (that was used to produce the water) to avoid bias (Mora and Theratest) to run these tests.

The spiral generator was tested by checking laser diffraction (this could be basically checked using a laser pointer) and found that the Northern hemisphere coil shifted the water to the left after treatment and Southern hemisphere water to the right.

In practice drinking one litre of energised water half an hour before breakfast induces a general improvement in well-being feeling and in particular seems to impart a detoxification. This shows in bowel movements which may be twice a day to start with and in skin improvements. It is interesting to note that the CEO of the large Chinese drug company stated at a Hong Kong Conference that 1 litre of water 30 minutes before breakfast was better than any drug.

Splitter Box

This is designed to enable up to 6 accessories to be permanently connected to the QXCI/SCIO output. They are then ready for immediate use thus reducing time and hassle in changing over between items.

Part 2: Program Facilities

Program Access Points

There is nothing magical or special about selecting the program aspects to use with accessories. Select the treatments as you would normally e.g. use both the appropriate pathogen and the healthy tissue sarcode, support the associated areas as well as dealing with the presenting infection etc. Understand the process leading to the dysfunction or disturbance and thus identify the possible treatments.

The principle of use is

1. Enable-activate the attachment.
2. Select the power: remove head harness if using double power.
3. Select the treatment that you want to pass through the probe.
4. Consider any underlying aspects that need action.
5. Consider making a remedy for the client,

The following screens have specific activation facilities:

Screen	Route	Notes	
Any	Provided that the output is activated ANY THERAPY can be output from ANY SCREEN.	ANY THERAPY	ANY SCREEN
Test	Treatments > Activate Point Probe	Point probe Active (top right of screen). The probe or roller will stay active for all subsequent treatments or therapies.	Zap of any item Zap from filter
	Treatments > Deactivate Point Probe	Deactivates the probe/roller	
Dental	Therapies	<i>Specific Therapies:</i> Cavity Zap Point Probe Restore tooth Point Probe Gingivitis Point Probe	<i>Other Therapies</i> Balance muscle Rx Trauma repair Rx Pain reduction Rx Nerval repair Rx
TMJ Muscles	Dental>TMJ Drop Down >Show TMJ Scan> Show TMJ Muscle Sarcode	Muscles	
Body Scan and Face Therapy	Test > Programs > Body Scan and Face Therapy > Skin Rejuvenation	<i>Specific Therapies:</i> Point Probe Warts Point Probe Spots Point Probe Lines Point Probe Cellulite	<i>Other Therapies</i> Breast Enlarger Hair, anti balding Anti Aging Detox Pulse Face Lift Neck Therapy Systemic Cellulite Forehead Treatment Eyes Treatment

			Chin Treatment Lips Treatment Overall face Tone
<i>Animals</i>	Test> Treatments > Animals	Specific pathogens.	
<i>Ears</i>	Test>Programs> Spinal and Sarcodes>Timed Therapies>Ears		
<i>Eyes</i>	Test>Programs> Spinal and Sarcodes>Timed Therapies Test>Programs> Spinal and Sarcodes> Eyes		
<i>Disease Lexicon</i>	Activate Point probe	Will then be active in all treatments	

Test Screen Facilities

Once activated any of the following treatments will pass via the attachment in addition to the harness. Thus in the test screen you can treat any item in the main test matrix.

There is no need to remove the harness-this will also deliver the treatment so that any other parts of the client that want some of the healing pattern will benefit. There will be treatment effect through both routes: the harness is not disabled.

To activate probe: Test > Treatments > Activate Point Probe.

To de-activate: Test > Treatments > De-activate Point Probe.

To set / reset power: System Power Settings

Within the test screen you can use the point probe for:

3 sec. treat

3 minute Zap

Zap list drop down

Use Search function to generate a list and the “Zap from Filter”.

Use colour code buttons (dental nosodes etc.) to generate a list and the “Zap from Filter”.

Remember that any therapy after the probe (or roller) is activated (e.g. spinal). This means that the roller can be used to go down the spine. The point probe can be used on specific acupuncture points.

Use whatever tool is appropriate to the size to be treated and select the power and time according to the client vitality, depth of the issue etc.: just as you would do normally.

Dental

Tools

Appropriate tools

Standard tip

Notes

Not recommended for inside mouth from hygiene considerations: use extensor.

Angled tip

Cavity zap, between teeth,

Extensor

Deeper in mouth, muscles, gingivitis, gum line.

Spoon

Tongue thrush etc, ulcers, cheeks
ulcers/thrush etc.

Treat according to nature of issue.

The request from dentists was the original thrust behind the development of the probe.

Access: TEST > Programs > Dental > Information > Start Info Exchange

Access is also possible from a number of other screens, where the dental button is displayed.

Functions Overview

- Dental Sarcodes (teeth), Isodes (materials), Nosodes (pathogens) transferred from the main test screen. (It is as easy and more flexible to treat in the main screen)
- Individual reaction and treatment of the above
- Acupuncture connection to teeth (Teeth tables)
- Dental Foci: various above neck areas and causal factor reactivities.
- Teeth Chart for testing and treating individual teeth
- Therapies for Balance muscle Rx, Trauma repair Rx, Pain reduction Rx, Nerval repair Rx: these work really well with the attachments.
- Specific therapy for teeth cavities (infection and restoration), gingivitis.

There are a suite of attachments to significantly increase the impact of dental therapy aspects.

Dental Therapies

Access Therapies (set time in min) on top toolbar

The top four items are not available until a therapy time has been set (see the top right of screen: use scroll bars to see if necessary). It is possible to add patterns (*Therapies>Piggy*)

Back Therapies). Some will be loaded on entry. Reset to clear and add your own, Load and then *close*. **Close may not work.**

Balance muscle Rx	Set timer to enable.
Trauma repair Rx	Set timer to enable
Pain reduction Rx	Set timer to enable
Nerval repair Rx	Set timer to enable
Add additional therapy to treatment	This does not seem to have any action
Double power	Doubles the intensity of treatment. Use with caution. Restore normal power after use or the higher power may still apply when you leave this screen.
Normal power	Return the power setting to normal: there is no display to this effect.
Cavity zap point probe (Note 1)	When connected to the rear of the interface box via the red banana plug, the treatment energy is directed down the point probe for one minute.
Restore tooth point probe (Note 1)	Rebuilds small tooth defects
Gingivitis point probe (Note 1)	Treats localised gingivitis
Point probe Treatment of item in main matrix(Note 1)	Allows for point probe treatment of any item in the main matrix: use the Load..from main for the full matrix list
Max Power, Warning use at own risk	Know why you are using this!!! Note the warning message. Restore normal power after use or the higher power may still apply when you leave this screen.

There is a Double and normal power selector: use with care and be aware that there is no message about which one is selected. Please be safe and just use normal power unless there is a specific need. The dental specific treatments will run for 1 minute and cover:

To treat any main matrix item select the item, then “Point Probe Amplification from main matrix”. The same process as above will ensue.

<i>Therapy</i>	<i>Attachment</i>	<i>Notes</i>
Balance muscle Rx	External: Pads, spoon Internal: extensor	Set timer for min.. 2, try 10 mins. Power x2
Trauma repair Rx	External: Pads, spoon Internal: extensor, angled	5-10 mins, power x2. Once per day. Use in combo with pain and nerval.
Pain reduction Rx	External: Pads, spoon Internal: extensor, angled	5-10 mins, power x2. As needed: continue 1-2 hours later if pain returns. Use in combo with trauma and nerval.
Nerval repair Rx	External: Pads, spoon Internal: extensor, angled	5-10 mins, power x2. Once per day. Use in combo with pain and trauma
Cavity zap point probe	Extensor or angled	This is 1 min. Rx. Use x5-10 according to severity. Daily for 7-14 days. x2 power
Restore tooth point probe	Extensor or angled	As for cavity zap. x2 power
Gingivitis point probe	Extensor on gums, angled between teeth	This is 1 min. Rx. Time according to severity. x2 power. Every 3 days till improvement.

All settings are just suggestions and should be adjusted according to child, elderly, vitality, severity etc. Monitor for patient discomfort/ alarm. If using head harness consider placing away from head e.g. abdomen (where there are as many brain cells!!)

TMJ Muscles

There are some 60+ muscles in the face: some of these are internally accessible and respond well to direct treatment by the probe. The user will need to do their own study to know where muscles are located.

Tools

The probe and extensor tip is recommended.

Test Screen facilities.

Use *Search and TMJ* to locate items. These include various ligaments and muscles as below. All the individual reaction, treat, zap and zap from filter aspects can be used. The *Load Report* function can be used to check remedy associations and the hold tray to review infection.

Cranial Bones Facial TMJ |
Ligament TMJ Capsular | Sarcode
Ligament TMJ Collateral | Sarcode
Ligament TMJ Peridontal Tooth Ligament | Sarcode
Ligament TMJ Spheno Mandibular | Sarcode
Ligament TMJ Stylo Mandibular | Sarcode
Ligament TMJ Temporo Mandibular | Sarcode
Muscle Facial TMJ Anterior Temporalis | Sarcode
Muscle Facial TMJ Deep Masseter | Sarcode
Muscle Facial TMJ Inferior Lateral Pyteroid | Sarcode
Muscle Facial TMJ Medial Temporalis | Sarcode
Muscle Facial TMJ Post Temporalis | Sarcode
Muscle Facial TMJ Superficial Masseter | Sarcode
Muscle Facial TMJ Superior Lateral Pyteroid | Sarcode
TMJ (DR) | Sarcode remedy
TMJ (NV) | Sarcode remedy
TMJ DISFUNCTION | MIASM-TET (DR) |

TMJ Muscles

This is a staged test. The patient is required to clench certain teeth on each of the 7 muscle exercises. Each muscle test is about 6 seconds. In each exercise the patient holds the position while you click the button. The patient may relax between the exercises. It may be beneficial to do the TMJ Scan and balance first. In particular the

Pterygoid muscle is important in that it affects the upper-lower jaw alignment: use the long probe attachment to reach and treat this specifically.

TMJ Drop Down > Show TMJ Scan > Show TMJ Muscle Sarcode
(If the screen does not show click on Show TMJ Scan)

Select Normal

1. Do the Muscle Balance Rx (*Therapy > Set Time > Balance Muscle*). Subsequent steps below will refine this.
2. Click *Start TMJ Scan*
3. Click *Clench Back Teeth* (client to clench back teeth)
4. When the next button appears do it (the windows interrupt may not disappear)
5. Repeat for all other items (with appropriate actions)
6. After the set is completed Click *Results* button that appears.
7. The results of difference between the muscle tension and the normal relaxed pattern are accessed by clicking the difference (e.g. DIF clenched back) buttons. This displays in a table below the value differences. These can be either negative or positive.
8. Treat an item if it is below -40/60 by double clicking on the name. The Windows Interrupt will display values that may be useful (see below). It is possible to add patterns (*Therapies > Piggy Back Therapies*). Some will be loaded on entry. Reset to clear and add your own, Load and then close. **Close may not work.**
9. Continue through all difference buttons. If an item has already been treated in an earlier panel then do not re-treat.

The results for each activity are shown after the activity together with the following information:

Resonance : 68 Reactivity : 90 Rectified : 41

The following also shows

Muscle tension : 61 Resonance : 56 Muscle Disease :5

Muscle tension indicates how much tension is held in the muscles associated with this area. The higher the number the higher the tension or tightness being. High numbers can indicate a tendency to spasm.

Sarcode resonance indicates how much resonance there is to the healthy energetic pattern at tissue/cellular level.

- Greater than 110-120 indicates over functioning, too much energy, probably healthy but stressed from an outside source.
- 50 to 80 is a good healthy range
- Under 50 can indicate under functioning with too little energy and the possibility of unhealthy or disturbed tissue.

Muscle disease with a high number indicates a disturbance but not necessarily intrinsic within the tissue. Especially if sarcode resonance is sound there is likely to be a secondary cause such as infection, trauma etc. i.e. it indicates an external source.

Pain

Tools

<i>Appropriate tools</i>	<i>Area</i>	<i>Notes</i>
Pain Pads	Small areas, joints	x2 power, till some resolution starts, repeat as pain recurs, also look for any chronic underlying.
Small mat	Larger pain area	As above

Program Facilities

Screen Access *Test Screen > Programs > Pain*

Beauty: Body Scan and Face Therapy

Tools

<i>Appropriate tools</i>	<i>Area</i>	<i>Notes</i>
Standard probe	small spots small warts lines	1 min, x2 power, x1-2 per day till resolving 2 min, x2 power, , x1-2 per day till resolving Use face analysis & QX program to determine what underlying aspects are relevant. Consider Rx from aging program. Use the standard tip or the extensor and run it gently along the lines. Try 2 min. per line, x2 power, x12 per day.
Extensor	lines, larger spots and warts	
Spoon	Larger blemishes	Treat according to nature of issue.
Std. Roller	Larger areas	Treat with slow rolling movements: x2 power.

Program Facilities

Screen Access *Test Screen > Body Scan and Face Therapy > Skin Rejuvenation*

The *Skin Rejuvenation* system will also allow a scan of foci and then it will allow several types of therapies for rejuvenation and detoxification. Set the time in minutes and start the therapy.

<i>Therapy</i>	<i>Attachment</i>	<i>Notes</i>
Point probe warts	Std. tip, spoon, extensor	Rx is 1 min. Try 2-5 mins, each 3 days till change. x2 power
Point probe spots	Std. tip, spoon, extensor	Rx is 1 min. Try 2-5 mins, each 3 days till change. x2 power
Point probe lines	Std. tip, extensor	Rx is 1 min. Try 2-5 mins, each 3 days till change. x2 power
Point probe cellulite	Std. roller. Cellulite roller.	This is for localised small areas. Rx is 1 min. For each area try 2-5 mins, each 3 days till change. x2 power. Brush towards lymphatics. Use lymphatic support, in QX and trampoline. Consider systemic cellulite as support.
Breast Enlarger	Roller, pain/beauty pads	2-5 mins, each 2-3 days. x2 power.
Hair, anti balding	Roller, pads	2-5 mins, each 2-3 days. x2 power ? Care since x2 power may induce headache indicating over treatment.
Anti Aging	Roller, pads	20 sec. Rx. Repeat x5-10. Each 3 days. x2 power ?
Detox Pulse	Roller, pads	20 sec. Rx. Repeat x5-10. Each 3 days. x2 power. Do lymph.

Face Lift	Roller, pads	20 sec. Rx. Repeat x5-10. Each 3 days. x2 power
Neck Therapy	Roller, pads	20 sec. Rx. Repeat x5-10. Each 3 days. x2 power ?
Systemic Cellulite	None	20 sec. Rx. Repeat x5-10. Each 3 days. x2 power ? Use as supportive to point probe cellulite.
Forehead Treatment	Roller, pads	20 sec. Rx. Repeat x5-10. Each 3 days. x2 power ? Care since x2 power may induce headache indicating over treatment
Eyes Treatment	Eye attachment	20 sec. Rx. Repeat x5-10. Each 3 days. Normal power.
Chin Treatment	Roller, pads	20 sec. Rx. Repeat x5-10. Each 3 days. x2 power ?
Lips Treatment	Spoon	20 sec. Rx. Repeat x5-10. Each 3 days. x2 power ?
Overall face Tone	Roller, pads	20 sec. Rx. Repeat x5-10. Each 3 days. x2 power ? Work on primary areas.

All settings are just suggestions and should be adjusted according to child, elderly, vitality, severity etc. Monitor for patient discomfort/ alarm. If using head harness consider placing away from head e.g. abdomen (where there are as many brain cells!!)

Whilst some of the treatments are specifically designed for the probe/roller/ pads connected to the QX probe outlet they can all be used with attachments provided the point probe facility is set to active in the test screen (*Test>Treatments>Activate Point probe.*) The attachments apply the pattern locally and thus enhance physical results.

Specific buttons for point probe warts, point probe spots, point probe lines, point probe cellulite will deliver 1 minute of therapy. Clicking any of the above buttons will initiate a “Point Probe Amplification Active” message panel. Click OK for a 1 minute therapy. The timer has no effect

Anti-aging and *Detox Pulse* require the timer to be set to be enabled.

Oriental Face diagnosis displays information for using facial disturbances for diagnosis. Use *Restore Face Therapy* to restore the previous panel.

Additional

Items loaded into the upper left edit boxes can be added to the therapy, so that these patterns will go out concurrently. Try to use words that correspond to the main test matrix descriptions.

Sarcodes are healthy tissue

Nosodes are diseased or infectious tissue

Allersodes are for allergy desentization

Isodes are for detoxification.

Add these to the therapy if you can.

Sarcodes and Short Sarcodes (Eyes and Ears)

General

Sarcodes are healthy tissue patterns: treating here addresses the foundational structure of the cells and thus tissues and organs. As such it deals deeply and the following are relevant:

- Correction may be slow: sarcodes are difficult to correct.
- It is better to treat in the Timed Therapies Panel rather than double clicking in the sarcodes table.
- Some aspects can also be located in the test matrix.
- If an issue corrects to above 60 ish. After 1 minute then it is unlikely to be an issue.
- Sarcodal treatment gives vitality to the organ/system: it may then start to detox on its own.
- Sarcodal therapy alone can be beneficial in reducing allergy reaction by enhancing tissue integrity.

Tools

The tools developed for these areas are specific.

Eyes

1. A twin unit with electronic non return to enable concurrent treatment of both eyes.
2. An attachment for the point probe that will treat each eye in turn.

Ears

The attachment is a conductive moulding.

1. A twin unit with electronic non return to enable concurrent treatment of both ears. (Available April 2004)
2. An attachment for the point probe that will treat each ear in turn.

Eyes: Main Treatment Locations

1. Main Test Screen: use search etc. to identify relevant items and then treat, zap or autozap from filter as normal.
2. Spinal and Sarcodes>Original Sarcodes> Timed Therapies
3. Short Sarcodes

Remember that the individual reaction will help to identify progress (via a reducing resonance value)

Sarcodes

Access Test>Programs> Spinal and Sarcodes>Timed Therapies

Test>Programs> Spinal and Sarcodes> Eyes

There are two (2) aspects:

1. The Timed Treatments table> Eyes (ears)
2. The buttons below that access specific areas: Eye (ears)

Remember that the individual reaction will help to identify progress (via a reducing resonance value)

Treatment Duration and Frequency

Duration: 2-5 minutes.

Frequency: each 2-3 days.

Power: **normal**

Basic Operation

On entry the screen will display:

- Client selected therapy (red highlight)
- Client selected piggy backs (red highlights)

You can accept or alter any of the above parameters. An option is to do the suggested therapy for 1 minute and then do your choice. It is possible to have the client second choice using “*Repeat Unconscious Choice*”.

Set time (1 minute to check if an issue and 5-10 minutes for treatment) and click Start: a rectified is returned on completion.

Subspace operation can be set via the “*Check for Long Undefined Therapy*”: at the expiry of the timer setting a new screen will display. Click *Close* when you want to finish the subspace aspect.

The timed therapies button will access a suite of sarcodal therapies. There are additional individual buttons for the group areas of muscles, bones, nerves, circulation, lymph, digestion, eye and sinus.

Essentially sarcodes are the energetic patterns of healthy tissues. Some of the patterns within the QX system may include associated nosodes. If a dysfunction has an organ focus then this is a valuable therapy. Health restoration involves identifying and eliminating the stressor and supporting the healthy function. When working on a dysfunction then sarcodal therapy offers a lateral approach. For a serious/difficult dysfunction an approach using a variety of angles is good.

On entry into all the sarcode treatment facilities the clients unconscious selection is highlighted, together with the associated piggybacks. There are measurements in each system for rectification. A good target is 85% or more. However for difficult issues rectification may not go above 40-50 for several visits. Sarcodes are intrinsically difficult

to correct since the work is at the base foundational level of the system. Rectification may go down, possibly reflecting a detoxification process. Don't be concerned.

Some practitioners will check an item for one minute to see what the rectification is and then draw a conclusion on the time needed. However the time required to effect rectification is not linear. However if an organ does correct to a higher rectification quite quickly it is a hint that the organ is basically healthy. Conversely if an organ does not correct well then it is an appropriate focal area. A general recommendation for time selection, in common with other therapies, is to try 5-10 minutes initially.

In all screens it is possible to select additional patterns to operate concurrently with the selected therapy. Adding many items may extend the treatment time considerably.

In some screens an alarm response will show in the screen with a message to double click to correct. If this does not clear or there is no facility then return to the test screen and use the Treatments>Alarm Correction Facility. If this does not correct the alarm either finish the session or use Biofeedback>Biofeedback>Treat Stress in Nerves to quieten the system.

Piggy backs- Additional Patterns

There are additional data for therapy boxes for the following items: the item names/terms used should be similar to those found in the test matrix. A double space is required between each different item.

Nosode, Isode, Allersode, Sarcode, Symptom

There are also additional treatment facilities available for:

Chinese aspect

Treat dryness in the area
Treat damp in the area
Treat cold in the area
Treat heat in the area
Treat wind in the area
Treat phlegm in the area
Treat energy stagnation
Treat weak chi
Adjust trivector disorders

General aspect

Treat pain in the area
Relieve inflammation in the area
Treat metabolic dysfunction
Treat injury in the area
Treat infection in the area
Treat degeneration in the area
Treat fibrous tissue in the area
Send detox pulse into the area
Release emotional stress

(Nosodes are diseased tissue, pathogens)

Isodes are materials (mercury, toxins)

Allersodes are homeopathic preparations designed to desensitise allergens)

Short Sarcodes

Access Test>Programs> Short Sarcodes

Basic Operation

Where there is a named part on the screen clicking on the name will activate a treatment. Clicking any other place will treat the whole aspect. Therapists have observed good results in working through the individual aspects.

There are five indicators of progress: as elsewhere the readings bounce about. QX suggest that a reasonable balance is >70% rectification and the inflammation etc. markers all below 40.

There is access via the left column radio buttons and via top tabs: see below.

In all screens it is possible to select additional patterns to operate concurrently with the selected therapy. Adding many items may extend the treatment time considerably.

In some screens an alarm response will show in the screen with a message to double click to correct. If this does not clear or there is no facility then return to the test screen and use the Treatments>Alarm Correction Facility. If this does not correct the alarm either finish the session or use Biofeedback>Biofeedback>Treat Stress in Nerves to quieten the system.

Short Sarcodes- Eyes

Eye Diagnosis + Rx

Eye Points	Acup points for eye
Eye anatom	Eye treatment facilities for: superior rectus muscle, sclera, retina, vitreous humor, anterior chamber, cornea, eyelid, optic nerve, visual cortex, inferior rectus, iris, conjunctiva, vitreous chamber, posterior chamber, lens, fovea centralis, optic chiasm, visual memory
Galucoma Pt Rx	Acup Rx points for Galucoma
Iridiology	Iridology chart, test and treat
Eye Anatomy	Rx for superior rectus muscle, Sclera, Iris, Cornea, lens, Anterior Chamber, Posterior Chamber, Conjunctiva, Interior rectus muscle, Optic nerve, Fovea Centralis, Retina, Vitreous Chamber
Eye Muscles	Rx for Superior Rectus Muscle, Superior Oblique Msucel, Medial rectus Muscle, Inferior Rectus Muscle, Inferior Oblique Muscle, Optic Nerve
Next Eye Pic	Series of Iridology pics. For various dysfunctions: see below.

Ear + etc.

Eye	Oriental Eye Diagnosis Info.
Eye muscles	Lateral rectus muscle, Superior Rectus Muscle, Levator palpebrae Superious Muscle, Superior Oblique Muscle, Medial Rectus Muscle, Inferior Rectus Muscle, Interior Oblique Muscle, Optic nerve

Short Sarcodes- Ears

Ear + etc.

Ear anatom	Pinna, Bone, External Auditory canal, Ear Lobe, Malleus, Eradrum, Semicircular canals, labyrinths, Auditory Nerve, Cochles, Eustchian Tube, Incus, Stapes, Oval window
Ear Acup	Antiaging, metabolic restoration
Ear back	Various ear points
Ear acu	Various acu points
Ear misc	Hearing stim acu pt.
Inner Ear	Cranial nerve, Cochlea, Ear drum, External auditory canal, external ear, hammer, Stirrup, Anvil, Semicircular canals.

Piggy backs- Additional Patterns

There are additional data for therapy boxes for the following items: the item names/terms used should be similar to those found in the test matrix. A double space is required between each different item: Nosode, Isode, Allersode, Sarcodes, Symptom, Misc

Aging Program

Access: *Test>Programs>Aging*

Testing and calibration are necessary to generate the values that display. It is suggested that Auto Therapy is done first.

Basic Operation

Anti Aging Belief Therapy, Anti Aging Relaxation Training, Anti-Aging Therapy, Anti-Aging Teliomere Repair generate audio visual presentations that can alter mind set, educate and relax. Click the “x” in the movie to close. Drag the bottom right corner of the movie to increase size.

Anti Aging Rx opens the main aging panel. This contains *reactivity* scores for the various factors associated with aging. The higher the value the more significant it is. Each item can be treated by clicking. If the item exists in the main test matrix it can also be Individual Reaction Tested and zapped from there.

Internal aspects that are relevant to aging shown are:

Telomeres of DNA	Growth Hormone	Calcium in Tissues
Strand	Releasing factor	
DHEA	Growth Hormone	Free Radicals
Melatonin	Elastin	Fatty acids Anti Aging
Parathyroid Hormone	Collagen	Messenger RNA
Growth Hormone	Thymus Hormone	

Target Values

Quantic Decay < 50

Energetic, Tissue and overall metabolic ages should be similar to the person’s real age.

All other items should score below the purple band in the main test matrix.

Main Matrix Items

The following of the above items are also available in the main test matrix, for doing longer treatments or an individual reaction

	<i>Main Matrix</i>		<i>Notes</i>
Elastin	583, 2537, 3879	104	Ave.
Telomeres of DNA	See also Biofeedback,		
Strand	DNA		
Melatonin	Item 5252	106	Fixed
DHEA	Item 5251	75	Fixed
Growth Hormone	1325, 2514	99	Floating
Releasing factor			

Growth Hormone	2531	75	Fixed
Parathyroid Hormone	2803, 1441, 2556	97	Fixed, ave.
Collagen	3873,5821	102	Floating
Thymus Hormone		111	Floating??
Calcium in Tissues		82	Floating??
Free Radicals		90	Floating??
Fatty acids Anti Aging		90	Fixed
Messenger RNA		99	Fixed

Causal and regenerative factors shown are:

Nelson Fatty Acid remedy for anti aging (only source of all fatty acids)
Premature Aging from Sun or perverse energy
 Emotional tension
 Toxicity or dehydration
 Virus

Energetic, Tissue and overall metabolic ages are also shown.

Other Therapy Places

- *Body Scan and Face Therapy>Skin Rejuvenation>Antiaging*
- *DNA Teliomere in DNA (via Auto trivector)*
- *Biofeedback>Organ Systems>Skin Stabilisation*
- *Biofeedback>Additional>Anti-Aging*

Animals

In order to test and treat animals the same entry formalities and general approaches apply as for us two leggeds. The same test and treat facilities can be successfully applied, including the use of virtual. Consider the QXCI suggested therapies as in “Client unconscious Choice of therapy” in Biofeedback etc.

Note that the animal pads are for treatment only. Testing for most animals is very sound in subspace.

The USA expert on Horses is Suzan Covington: I thoroughly recommend any of her trainings.

Considerations specific to animals

In addition to the standard test and therapy options there are some animal specific facilities for:

- General health parameters and possible origins of dysfunction
- Specific isodes and nosodes
- The most appropriate homeopathic of an isode or nosode
- Dietary balance/nutritional intake
- 20 second treatment of the animal specific items.

Access

The main location is:

Test>Programs>Cranial Sacral/Relexology/Animal>Animal Reactions.

Note that Animal Reactions will only show if you have set animal type via demographics.

There is also a catdog.bmp facility in Acupictures

Pre-requisites

Ask permission of the animal.

Demographics>Select animal testing: either the button or Demographics drop down>Animal Testing.

Select the most appropriate animal, click “Load and Close”

Enter name, birth date and all other data as normal. If you do not have an exact birth date put the nearest: the exact is important for Biorythms but intent is the most important. If it helps your intent to focus put a little of the hair of the animal into an envelope without touching it and use on the test tray.
Run calibration, test etc. as normal.

Harness Connection: connect the head harness to the abdomen, and the straps to the limbs. For horses there is a special bridle that accepts the head harness. For all 4 legged's there is a quick break connect facility. (Contact QX or Broker).

Alternatively put the headband around the belly of the animal: the headband will do input and output if the straps are absent. It can be made longer with a belt, Velcro strap etc.

Specific Considerations for Horses

User experience indicates that subspace is good for testing as animals have a very clean energy field and access is good. If I do my cats subspace they will often come and seek me out! For young active animals this may be the safest option for expensive equipment. Cats and horses are very sensitive to electromagnetics, so be aware of duration. Some animals have had bad experience of shots etc. and may not like being restricted. My cats get up and go away if I run too long and then may come back and lie on the pad.

Calibration, Testing, Interpretation, Therapies: Proceed as normal.

Basic Operation

The animal categories covered are:

- Cat (feline)
- Dog (canine)
- Horse (equine)
- Cow (bovine)
- Other mammal (specific aspects for goat, sheep, turkey, pig)
- Cold blooded (snakes etc)

The initial screen is the equivalent to the human dental foci screen described above and will display the same value. The tabs along the top of this panel relate to various animals and bring up various criteria specific to each animal.

These reactivity values are derived from specific animal nosodes, isodes and sarcodes. They are not accessible from other screens. The potency button has nothing to do with the nutrition panel. It is here to be accessible to all the individual animal screens in selecting the nosode/isode potency:

General Screen

This is used in the same way as its dental look alike. There are essentially two areas to this display.

Physical foci

Potential causes

The physical foci categories are:

Physical foci

Drainage: tonsils, sinus, lymph

Bone: jaw, TMJ, cranium

Circulation: bacterial, venous

Muscles

Hormonal

Nerval : motor, sensory, sympathetic, parasympathetic

Gums

Potential causes

Infection

Toxicity

Trauma

Radiation

Allergy

Deficiency syndrome

Stress

The numbers are initial reactivities. The higher the score the more significant is the item. Thus a high score indicates tonsils under drainage and infection would indicate that tonsils are stressed via an infected agent. Since animals will have a low SOC numbers above 85 (here and here only!) are likely to be significant.

Nosodes and Isodes

Feline

Feline rhinotracheitis

Lennocel (len case feline)

Cat flu comb

Feline leukaemia

Cat enteritis

HIV feline

Loryza du Chat

HIV feline

Feline haer

Feline flu

Cat flu combo

Feline rhinotracheitis

Feline enteritis

Feline respiratory infection

Feline intestinal infection

Feline skin infection

Feline malabsorption syndrome

Feline psychological disorder

Feline cardiovascular disorder

Canine

Canine sensory disorder

Canine caudal disorder

Canine nerval disease

Canine cardiovascular disorder

Parvo virus

Distemper

Hepatitis – canine

Canine placenta

Canine sinus pus

Hard pad

Canine ferunculosis

Kennel cough nosode

Canine respiratory infection

Canine intestinal infection

Canine psychological disorder

Canine malabsorption

Equine

Equine cardiovascular disorder

New Forest eye

Horse fluid

Bovine (cow)

Bovine malabsorption

Bovine intestinal infection

Bovine respiratory infection

Equine respiratory infection
Equine intestinal infection
Equine malabsorption syndrome
Equine psychological disorder
Equine muscle disorder
Equine ligament disorder
Equine hormonal disorder
Equine nerval disorder
Equine lymph drainage disorder

Bovine cardiovascular disorder
Bovine hormonal disorder
Bovine immunity disorder
Bovine muscular disorder
Bovine connected tissue disorder
Bovine nerval disorder
Bovine mucus disorder
Bovine psychological disorder

Other Mammal

Foot rot (goat)
Sheep foot rot
Turkey vulture
Pig scabies
Rhinothacheitis calici virus
Virus caree
Myxomatosis
~~Virus caree: duplicate of above~~
Cardiovascular disorder
Psychological
Malabsorption

Cold Blooded

Cardiovascular disorder
Psychological disorder
Hormonal disorder
Nerval disorder
Muscular disorder
Intestinal disorder
Immunity disorder
Infection
Skin disorder

Treatment

Any therapy anywhere in the QX can be used on animals.
20 second Rx of last clicked item.

Click on an item in any of the screens except general (with the exception here of Foot and Mouth Disease 2001) to load the item into the bottom hold tray (Reset Homeopathic to clear the box) or several.

Then click on the *20 sec... button* for an energetic treatment.

Potency Scan

Despite being located on the nutritional intake panel this has nothing to do with animal nutrition. It is located there to enable it to be on view in each of the animal screens.

1. Click on the *nosode* or *isode*.
2. Click on *potency scan*
3. The potency to give as a homeopathic for that item will be displayed under the Potency Scan button.

Nutritional Intake

A small yellow panel displays in all screens giving nutritional intake in terms of:

Protein
Carbohydrates

Fats
Water
Minerals

Values will show on entry to the animal screens i.e. when the Animal Reaction button is clicked. Whilst the nutritional intake yellow screen may be available on entry into the cranial sacral and other info screen there are no values associated with it on entry.

If the values are about the same then the nutritional intake is balanced. Values above 80-90 indicate a potential deficiency. This aspect is particularly to pets which are fed with table scraps or human type food e.g. burgers!

Part 3: Remedy making and Importation

Introduction

The QXCI/SCIO has facility to both import remedy patterns and to export patterns (for connections see below). The Potentiser is intended to optimize these processes by communicating with the sample itself. The QXCI/SCIO has a test tray on top: this comparatively can be viewed as more of a broadcast facility: the pattern intake/output can be considered a broader and more dispersed pattern. There is also the possibility of interference from the interface internal electronics themselves in a subtle way. Neither of these effects is likely to be dramatic and the potentiser is designed to optimize the interaction.

The potentiser is specifically designed for solutions: the tip will enter the solution directly. There is also a tray element in case “sac lacs” lactose capsules are used: however it is suggested that these are made from a potentised solution.

It is possible to:

1. Export any item from the Test matrix
2. To export as the matrix potency (approx. 30x) or to alter the potency via the Homeopathic activation panel.
3. To export at any selected potency a homeopathic from the Homeopathic Activation Panel.
4. To export any treatment pattern (including Disease lexicon) from the QXCI/SCIO: for example if treating a client it is possible to export the pattern for degeneration or any zaps or auto treatments etc. into a remedy in order to provide the client with ongoing treatment. This can occur simultaneously with therapy or be a supportive selective remedy. This may be particularly appropriate for a client that you are working with in subspace.
5. So that the pattern does not pass through the container wall thus optimising for plastic containers.

Important Notes:

1. ALWAYS include organ support and drainage when giving a detox or zap type remedy. If you do not understand what is involved look at Heel/Rekeweg combination remedies or learn some basic homeopathy.
2. Ensure that the client has the resources to support the process that a homeopathic will initiate: intrinsic vitality, nutritional substances. For example it is dangerous to homeopathically stimulate mercury detox. if there are not physical substances present to chelate released mercury.
3. Be lateral and inventive: ANY treatment from the QX can be exported into a remedy.

4. The client does not need to be present: however if using the auto treatments rather than just exporting a remedy it may be more matched to the client to run the calibration and test before making the remedy.
5. It is possible that the initial pattern is the strongest in the remedy. Water will hold a vast amount of information so you can in principle export a complete treatment in a bottle.
6. When making a remedy without the client present then use double or max. power: this is felt to have a beneficial effect in the activity of remedies.
7. You can set the probe outlet in the test screen for all therapies from that time on to be output via the attachment as well as the harness: thus it is possible (but perhaps not recommended as the client will have moved on after the treatment and have different needs). It will not be possible to use max power (which is felt to have a beneficial effect in the activity of remedies).
8. The Narayani remedies may be especially good for general issues: there is a Materia Medica available for this (cost on application)

Within the test and dental screens it is possible to direct output to the point probe for any item in the test matrix. Within dental and Body Scan/Face Therapy specific therapies are available.

Some areas of application include:

Safety Note re Power Settings

The double power facility in the main test screen and dental has an effect on the output. Please be safe and use appropriately.

DO NOT use max. power with the client in harness when optimizing a remedy.

The power output can be segregated to the tray/output and isolated from the client (even with client connection)

Is the harness also active

The harness continues to stay active when the probe is active. The wave form goes through both outputs. Since the QX is putting out low energy wave forms, mainly of homeopathics, then the power is not reduced in the head harness channel. The inputs and auto-focus continues to operate. There is no need to remove the harness-this will also deliver the treatment so that any other parts of the client that want some of the healing pattern will benefit. There will be treatment effect through both routes: the harness is not disabled.

Remedy Making

Preparation

1. Connect the potentiiser.
2. Prepare a carrier solution as 20% alcohol/water. The alcohol can be good quality spirits. Alcohol is there for sterility and also will enable the pattern to hold better and for longer. Alcohol is also believed to facilitate holding of higher dimensional information and thus may be particularly appropriate for the emotional, metal, spiritual programs.
3. Place the remedy bottle under the tip so that the tip enters the solution.
4. Place an isolating pad (card/ rubber under the bottle to isolate it from the tray (if you have a mark 2 unit).

For some background see the text from the Clasp32 / Programs folder: duplic. This can be accessed via word or Windows Explorer.

Client in Harness- concurrent remedy and therapy.

1. Test> Power Settings> Double Power (optional)
2. Treatments>Point Probe Activate (this activates the red output)
3. Programs>Homeopathic Activation> Clear Carrier (this button is on the right hand top of panel: it may be difficult to view on 2003 software at screen resolutions less than 1280x1024). Do twice.
4. Programs>Homeopathic Activation> Energise Water (this button is on the right hand top of panel: it may be difficult to view on 2003 software at screen resolutions less than 1280x1024). Do twice. This puts a generally beneficial healing pattern into the water.

OR

5. Test> Treatments> Energise Water from QXCI Devices/Point Probe. Do twice. This puts a generally beneficial healing pattern into the water.
6. Any treatment that you run will now be output into the remedy only.

Note: If for any of the above operations you want the pattern in the remedy only then Test> System Power Settings> Activate Test Tray will disable the harness and virtual aspects and only the test tray and red outlet will be active.

Client in Harness- remedy making only

1. Test> System Power Settings> Activate Test Tray will disable the harness and virtual aspects and only the test tray and red outlet will be active. Thus the remedy only and not the client will receive the pattern.
1. Test> Power Settings> max. power.

2. Treatments>Point Probe Activate (this activates the red output)
3. Programs>Homeopathic Activation> Clear Carrier (this button is on the right hand top of panel: it may be difficult to view on 2003 software at screen resolutions less than 1280x1024). Do twice.
4. Programs>Homeopathic Activation> Energise Water (this button is on the right hand top of panel: it may be difficult to view on 2003 software at screen resolutions less than 1280x1024). Do twice. This puts a generally beneficial healing pattern into the water.
5. OR
6. Test> Treatments> Energise Water from QXCI Devices/Point Probe. Do twice. This puts a generally beneficial healing pattern into the water.
7. Any treatment that you run will now be output into the remedy only.

Client not present

1. It is necessary to have the QXCI/SCIO interface connected and powered up.
2. Calibrate as a minimum if you are exporting a treatment pattern. Treatment is optional.
3. If just making a remedy from a matrix or homeopathic screen item then calibration is optional.
4. It is optional and according to your belief system if you place a sample of the client (hair, photo etc. on the QXCI/SCO test tray).
5. Proceed as above.

Alternative via Stimulate Reaction/Duplicate Remedy

This facility is really covered by the other options: it is included for completeness.

1. Set up power etc. as standard.
2. TEST / Treatments/ *Stimulate Reaction-Duplicate Remedy*
3. In the display the top half of the screen is for Stimulate Reactivity. The lower half is for adding a remedy and for duplicating a remedy.
4. Type the remedy name in the "Enter Name of Item" edit box.
5. Select the destination if you wish to isolate the client.
6. Click

Invert from matrix

Amplify fro matrix

According to the effect that you want (normally amplify).

Amplify Pattern probably increases the pharmaceutical effectiveness. It may give a stronger pattern, cleaner or clearer. A hand made remedy will for example have a clearer pattern than a machine succussed one. This may be away to improve the clarity.

Invert Pattern when making a remedy from a QXCI/SCIO stored pattern is not appropriate UNLESS you may want to stimulate a client experience of an allergen etc! because everything in the matrix is there as a homeopathic. See remedy making below for appropriate use.

Making remedies from the Main matrix: at matrix potencies

1. Set up interface as above.
2. Select the item from the test matrix.
3. Click Treat twice for 2x3 second treatments or according to your knowledge/experience.

Making remedies from the Main matrix: with selected potency.

This uses the homeopathic activation screen.

Selecting a potency.

If you are not homeopathically experienced then PLEASE respect that the potency is important: selecting too high a potency may create effects that you are unaware of. More is not better: higher potencies are not necessarily better. The important element is potency selection is the appropriate potency for the client. The potencies in the test matrix are safe.

The homeopathic activation screen can be used for potency selection and checking as well as for making a homeopathic. There are items in the Homeopathic Activation Screen that are not in the main test matrix, notably classical homeopathics. For full information see the Homeopathic Activation Advanced Chapter (available via John Kelsey).

The harness/ Tray Output etc. selection facilities are also selectable in the Homeopathic Activation Screen. Particularly there is facility to:

Invert

Amplify

Amplify Pattern probably increases the pharmaceutical effectiveness. It may give a stronger pattern, cleaner or clearer. A hand made remedy will for example have a clearer pattern than a machine succussed one. This may be away to improve the clarity.

Invert Pattern when making a remedy from a QXCI/SCIO stored pattern is not appropriate UNLESS you may want to stimulate a client experience of an allergen etc! because everything in the matrix is there as a homeopathic. See remedy making below for appropriate use.

Testing for Potency of a Main Matrix Item.

1. Note the name of the item in the main test matrix.
2. Open the Homeopathic Activation screen: Test>programs>Homeopathic Activation.
3. Type the remedy name in the *Master Edit Box* (top left).
4. EITHER
 - a. Enter the potency in the “Type in Potency” box, click “*Test Reaction of Remedies*” and select a potency that shows 100% only. (This benchmark is based on experience). Note that if you do repeat testing for the same remedy that after the third attempt the client response will be dulled: the organism will get fed up! Do a different remedy and return.
 - b. Pre 2003 potency scan: note that pre Jan 2003 the feedback is that the *Access Scan for Potency* is not an accurate facility.
 - c. Jan 2003: *Load Homeopathic Remedy List*> double click on name in the Homeopathic list to load into the Potency test facility OR type in a name > *Check Potency*: this will display a potency. Click *Zap + Duplicate* to export, having integrated the standard previous steps for power, carrier clear etc.

Testing for Potency of a Homeopathic Activation remedy

1. Open the Homeopathic Activation screen: Test>programs>Homeopathic Activation.
2. *Click>Load Homeopathic Remedy List*
3. Double click on name in the Homeopathic list to load into the Potency test facility OR type in a name
4. EITHER
 - a. Enter the potency in the “Type in Potency” box, click “*Test Reaction of Remedies*” and select a potency that shows 100% only. (This benchmark is based on experience). Note that if you do repeat testing for the same remedy that after the third attempt the client response will be dulled: the organism will get fed up! Do a different remedy and return.
 - b. Pre 2003 potency scan: note that pre Jan 2003 the feedback is that the *Access Scan for Potency* is not an accurate facility.
 - c. Jan 2003: *Load Homeopathic Remedy List*> > *Check Potency*: this will display a potency.
5. Click *Zap + Duplicate* to export, having integrated the standard previous steps for power, carrier clear etc.

Multiple remedies

This can be effected EITHER

1. Sequentially: just follow the appropriate steps for each item.

OR

2. Concurrently:

- a. From Main Matrix: this is effected via the Info grid.
 - i. Test>Information>Empty Info to start new > accept are you sure.
 - ii. Drag and drop the desired remedies into the Info Grid.
 - iii. Test>Programs>Homeopathic Activation
 - iv. Load program from Info (topish left of screen)
 - v. Alternatively type in the remedy name, leaving a double space between each item. (Frequencies, codes etc. can also be used here: including Rife/Clarke frequencies)
 - vi. Testing for potency of a multiple remedy is not appropriate.
 - vii. Do relevant standard steps and then “*Start Therapy or Duplication*”
- b. Within Homeopathic Activation:
 - i. Load Homeopathic remedy List.
 - ii. Double click the relevant items: since the Master Edit Box will only take a certain number of characters edit out the descriptive text.
 - iii. Alternatively type in the remedy name, leaving a double space between each item. (Frequencies, codes etc. can also be used here: including Rife/Clarke frequencies)
 - iv. Testing for potency of a multiple remedy is not appropriate.
 - v. Do relevant standard steps and then “*Start Therapy or Duplication*”

Importing remedy patterns (into the Test Matrix)

Function To add a homeopathic, herbal remedy or supplement which is not in the test matrix

to it.

Access TEST > Treatments >Add Remedy to Matrix

Result A display panel. The top half of the screen is for Stimulate Reactivity. The lower half is for adding a remedy.

Procedure

1. Type in the name of the remedy as you wish it to appear in the test matrix (This need not be the full name but should be something that identifies it clearly.
2. The Take Pattern from test tray will change from shadow to bold
3. Select “Activate Test Tray”
4. Click on “Take Pattern from test tray”
5. The VARHO windows interrupt panel appears
6. After 30 secs or so the bar chart below the Edit box will display the trivector status of the entries. If the entry is not satisfactory then there may be a “Please Repeat

Process” message. Even if the Repeat message does not show if the 3 trivector bars do not have a good amount of fill take the cursor to the end of the remedy name entry box and click: this will reactivate the “Take Pattern from test tray”. Repeat until the bar are say 70%+ filled with blue.

7. The “Add Item to Matrix” Button appears. Click.
8. The “Edit Empty Lines” dialogue panel appears.
9. Select the line for your entry and click “Edit Name”.
10. Enter the name in the dialogue box exactly as the earlier entry
11. Click “OK”
12. The item name appears in the table. Click on “Save Name”
13. Click “Close” to return to the previous screen.
14. Close that screen to return to the Test screen
15. Activate the Retest drop down list and click on Virtual Test. This completes the process.

The VARHO windows interrupt panel appears.

You now need to check that you have a good pattern. Select the imported item in the main test matrix. Click on expand name > see the trivector picture for the remedy > chart to get the picture. If this says “Weak cohesive energy present” then the import is poor. If it says “covalent energy present” it is good.

Remedy Duplication

There are two routes

- Route 1: Test> Treatments > Stimulate Reaction/ Duplicate Remedy.
- Route 2: Homeopathic Activation.

Test Screen (remedy duplication)

To energetically duplicate energetically an external remedy.

1. Set up power etc. as standard.
2. TEST / Treatments/ *Stimulate Reaction-Duplicate Remedy*
3. In the display the top half of the screen is for Stimulate Reactivity. The lower half is for adding a remedy and for duplicating a remedy.
4. Type the remedy name (what it is called) in the “Enter Name of Item” edit box.
5. Select the destination if you wish to isolate the client.
6. The next aspects are two-stage: first import the pattern to a holding location and then export it to the client.
7. For a toxic, allergic etc. item

Click

Invert from Test Tray: if you wish to invert the pattern of a real substance to produce a cancellation pattern for the client Examples

are REAL allergens, pathogens, toxins etc. This will import the pattern to a temporary holding location (clipboard).

Then click *Duplicate* to tray/all according to destination requirements.

8. For a beneficial item (homeopathic, to stimulate the client to a good food so that they will energetically recognize it:

Click

Amplify from Test Tray to import the energetic pattern of the item. . This will import the pattern to a temporary holding location (clipboard).

Then click *Duplicate* to tray/all according to destination requirements.

Amplify Pattern probably increases the pharmaceutical effectiveness. It may give a stronger pattern, cleaner or clearer. A hand made remedy will for example have a clearer pattern than a machine succeeded one. This may be away to improve the clarity.

Invert Pattern when making a remedy from a QXCI/SCIO stored pattern is not appropriate UNLESS you may want to stimulate a client experience of an allergen etc! because everything in the matrix is there as a homeopathic. See remedy making below for appropriate use.

Homeopathic Activation Screen (remedy duplication)

To energetically duplicate energetically an external remedy.

1. Set up power etc. as standard.
2. TEST > Programs > Homeopathic Activation
3. The next aspects are two-stage: first import the pattern to a holding location and then export it to the client.
4. For a toxic, allergic etc. item
 - i. Click
 1. *Invert Pattern*: if you wish to invert the pattern of a real substance to produce a cancellation pattern for the client Examples are REAL allergens, pathogens, toxins etc. This will import the pattern to a temporary holding location (clipboard).
 2. *Take Energy in from Tray*
 3. Select a potency if desired
 4. Test the *Reaction of Remedy* if desired.
 5. Select destination (Tray to isolate client)
 6. Then click *Duplicate Homeopathic*.

5. For a beneficial item (homeopathic, to stimulate the client to a good food so that they will energetically recognize it:
 - i. Click
 1. *Amplify Pattern* to import the energetic pattern of the item. . This will import the pattern to a temporary holding location (clipboard).
 2. *Take Energy in from Tray*
 3. Select a potency if desired
 4. Test the *Reaction of Remedy* if desired.
 5. Select destination (Tray to isolate client)
 6. Then click *Duplicate Homeopathic*.

Amplify Pattern probably increases the pharmaceutical effectiveness. It may give a stronger pattern, cleaner or clearer. A hand made remedy will for example have a clearer pattern than a machine succussed one. This may be away to improve the clarity.

Invert Pattern when making a remedy from a QXCI/SCIO stored pattern is not appropriate UNLESS you may want to stimulate a client experience of an allergen etc! because everything in the matrix is there as a homeopathic. See remedy making below for appropriate use.

Other Program Access Points

Whilst the Test screen enables you to set up the export to the Potentiser the following other specific access points are included for completeness

The principle of use is

1. Enable-activate the attachment.
2. Set the power level
3. Select the treatment that you want to pass through the probe.

The following screens have specific activation facilities:

Screen	Route	Display
Test	Treatments / Activate Point Probe	Point probe Active (top right of screen). The probe or roller will stay active for all subsequent treatments or therapies.
	Treatments / Deactivate Point Probe	Deactivates the probe/roller
Dental	Therapies	Specific Therapies: Cavity Zap Point Probe

		Restore tooth Point Probe Gingivitis Point Probe
Body Scan and Face Therapy	Test / Programs / Body Scan and Face Therapy / Skin Rejuvenation	Specific Therapies: Point Probe Warts Point Probe Spots Point Probe Lines Point Probe Cellulite
Disease Lexicon	Activate Point probe	Will then be active in all treatments

Test Screen Facilities

Once activated any of the following treatments will pass via the output in addition to the harness.

- Treat (select 3 sec or 3 min via Zap/Unzap as always) - set the point probe under Treatments drop down.
- Zap Mode List-this has 6 items from the bottom “Point probe Zap active”
- Energise Water (Treatments/Energize water from QXCI/point probe). There is also now available a coil that will impart “spin” to the water.
- It is possible to treat any main matrix from the dental program as well. See 5.2.

Dental

The request from dentists was the original thrust behind the development of the probe.

Screen Access Test Screen / Programs / Dental

On access there will be a message “You Must start Info Exchange First”
Go to Information drop down, click on this and the “Start Info Exchange”. This loads the scores from the test matrix into the dental screen. There is no “windows interrupted” message and thus no re-testing occurs at this point.

Point Probe Access Therapies drop down list

This accesses both some specific dental treatments and the facility to use the point probe on any item in the main test matrix.

There is also a Double and normal power selector: use with care and be aware that there is no message about which one is selected. Please be safe and just use normal power unless there is a specific need.

The dental specific treatments will run for 1 minute and cover:

Cavity Zap Point Probe: treats the infective agents

Restore tooth Point Probe: facilitates small cavity repair

Gingivitis Point Probe: treats gum disease

For dentists there are some special tools (1 cm diameter flat disc, sharper point probe, hoop which can go right around a tooth) which attach to the probe tip. Be aware of local legislation which may restrict what you are allowed to do or claim.

Click on the topic from the list: a message will appear. Click OK. The therapy will run for 1 minute with a windows interrupt message. The mouse will freeze.

Part 4: Product Information

Probes and Rollers

These connect into the red socket on the QX interface to direct a healing pulse direct to a focal area. In normal use the treatment waveforms are sent to the patient through the head harness. The energy must travel through the body to be used where it is needed. Localised treatment is possible when the head harness is placed near a focal area e.g. for the treatment of Fibrositis in the shoulder or a lesion when using the degeneration program. Using in conjunction with the head harness amplifies the treatment efficacy. Within the test and dental screens it is possible to direct output to the point probe for any item in the test matrix. Within dental and Body Scan/Face Therapy specific therapies are available.




Some areas of application include:

Probe	Roller
Dental: Infection	Cellulite
Small cavity repair assist	General facial
Gingivitis	Muscles
Oral thrush/ulcers	
General: any item from the test matrix (3 sec or 3 min zap)	Warts
Mouth and tongue ulcers	Aging lines
Warts	
Any item in the test matrix	Any item in the test matrix
Any therapy after the probe is activated in the test matrix	Any therapy after the probe is activated in the test matrix

The harness continues to stay active when the probe is active. The wave form goes through both outputs. Since the QX is putting out low energy wave forms, mainly of homeopathics, then the power is not reduced in the head harness channel. The inputs and autofocus continues to operate. There is no need to remove the harness-this will also deliver the treatment so that any other parts of the client that want some of the healing pattern will benefit.

Oral use of Point Probe

These are designed to screw into the KB probe. They are silver plated and can be used for external or internal treatment.

Attachment D1	Used for flat tissue surfaces (tongue, cheek). Thrush. Herpes. Any topical application.		
Attachment D3	Spot surfaces: long and 3mm diameter to access oral internal muscles, round ended for scars, lines etc.	 4 mm diameter 70 mm long	
Attachment D5	A longer angled unit to give better access allowing a postreior approach e.g. into gum pockets.	 60 mm long	

Pain Pads

- splitter box with internal enhancement coil
 - (8) 2cmx2cm pads to be applied to the skin
 - technician can use
- Specific Applications*
- ✓ Localized pain
 - ✓ Joints, esp. small joint
 - ✓ Multipoint beauty therapy.

Eye Treatment Accessory

- Allows direct application to eyes
- Ideal for
 - Short sarcodes
 - Sarcodes
 - Eye nosodes etc. from Test matrix

Pet-Baby-Large Area Pad

- Special conductive rubber
- Lightweight and fluid resistant.
- Lie baby/ pet on

(Large sizes on request)

Specific Applications

- ✓ Babies
- ✓ Pets (they will walk away when they have had enough and may come back for more)
- ✓ Strap on for larger areas (back pain, muscles etc.)

Cream Maker

- This enables pattern export for client to topically apply.
- Export a pattern into an aqueous cream.
- Potentise the cream as for water
- Export any therapy pattern

Specific Applications

- ✓ Ideal for skin issues, beauty etc.
- ✓ Elastin and Collagen cream for anti aging.
- ✓ Try with the new breast enlarger button!

Cellulite Roller

- Ideal for Cellulite
- Lymphatic Massage
- Heavy Duty
- Large muscle applications

Specific Applications

It is tailored to assist weight management and cellulite reduction.

- ✓ Heavier Cellulite Areas
- ✓ Muscle

Water Energiser Coils

These are in the shape of a coil to facilitate both left spin and right spin patterns, as an overlay on the ordinary energise water pattern. Right spin is intrinsic to health. The coil acts as a spin amplifier and correction facility. The spin varies between the Northern and Southern hemisphere. Perrier or Lourdes water, which carry particular energetic patterns because of their molecular structure, produced in the Northern hemisphere may not have benefits in the Southern hemisphere.

The spiral generator was tested by checking laser diffraction (this could be basically checked using a laser pointer) and found that the Northern hemisphere coil shifted the water to the left after treatment and Southern hemisphere water to the right.

In practice drinking one litre of energised water half an hour before breakfast induces a general improvement in well-being feeling and in particular seems to impart a detoxification. This shows in bowel movements which may be twice a day to start with and in skin improvements. It is interesting to note that the CEO of the large Chinese drug company stated at a Hong Kong Conference that 1 litre of water 30 minutes before breakfast was better than any drug.